

Research Article

Spine3d: Evaluation of Deformity in Patients with Idiopathic Scoliosis: A Case Series

Mazza Daniele^{1,3*}, Gagliardo Salvatore², Barbarino Manfredi¹, Bolle Gabriele¹, Emanuele Giovanni¹, De Carli Angelo², Santoriello Vincenzo³, Febbi Massimiliano^{4,5}

¹Istituto Dermopatico dell'Immacolata, Via dei Monti di Creta, 104, 00167 Roma RM, Italy

²Orthopaedic Unit and Kirk Kilgour Sports Injury Center, S. Andrea Hospital, University of Rome "Sapienza", Via di Grottarossa 1035-1039, 00189, Rome, Italy

³Catholic University, Milan, Italy

⁴ASOMI College of Sciences, School of Medicine, Head Office: Navi Building, Pantar Road, LJA 2021, Malta, Educational Campus: Giorgio Mitrovich Street, Pembroke, Malta, School of Medicine: Triq Is Sirk 121, Swieqi, Malta

⁵Laboratory for Rehabilitation Medicine and Sport (LARMS), Rome, Italy

*Correspondence author: Mazza Daniele, Istituto Dermopatico dell'Immacolata, Via dei Monti di Creta, 104, 00167 Roma RM, Italy and ASOMI College of Sciences, School of Medicine, Head Office: Navi Building, Pantar Road, LJA 2021, Malta, Educational Campus: Giorgio Mitrovich Street, Pembroke, Malta, School of Medicine: Triq Is Sirk 121, Swieqi, Malta; Email: daniele.mazza@hotmail.it

Citation: Mazza D, et al. Spine3d: Evaluation of Deformity in Patients with Idiopathic Scoliosis: A Case Series. J Ortho Sci Res. 2024;5(3):1-8. <https://doi.org/10.46889/JOSR.2024.5312>

Received Date: 11-11-2024

Accepted Date: 25-11-2024

Published Date: 02-12-2024



Copyright: © 2024 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CCBY) license (<https://creativecommons.org/licenses/by/4.0/>).

Abstract

Idiopathic scoliosis is a complex orthopedic condition marked by a lateral spinal curvature, typically affecting children and adolescents. The Cobb angle is a key metric for evaluating scoliosis severity through X-rays, but its measurement can suffer from variability due to imaging quality, positioning and physician experience, with an acceptable range of variation up to 5 degrees. LiDAR technology offers advantages over traditional methods, as it eliminates ionizing radiation and provides precise three-dimensional representations of the body. This study aims to assess the accuracy and reproducibility of Spine3D, a LiDAR-based tool, in measuring the Cobb angle in idiopathic scoliosis patients.

This study, conducted at Sant'Andrea University Hospital in Rome from September 2022 to September 2024, focused on adolescents (ages 10-18) with idiopathic scoliosis, excluding those with secondary curves or relevant health issues. Informed consent was obtained and body metrics were recorded. The Spine3D system, utilizing infrared technology for non-invasive spine assessment, measured alignment and generated detailed reports on parameters such as the Cobb angle and spinal curvature. Out of 29 participants, 26 were analyzed, showing an average Cobb angle of 29.9 degrees. Results indicated measurements of shoulder asymmetry, pelvic tilt, kyphotic and lordotic angles, with no significant statistical variations observed.

The measurement of the Cobb angle using Spine3D has demonstrated excellent reliability and efficiency. It is therefore suggested to promote the use of this method in clinical practice, alongside radiographic monitoring. Further studies will be needed to evaluate the spinal curvatures measured using Spine3D and traditional radiology.

Keywords: Idiopathic Scoliosis; Radiographic Monitoring; Spine; X-ray

Introduction

Idiopathic scoliosis is one of the most complex orthopedic conditions, characterized by a lateral curvature of the spine without a defined cause. It predominantly affects children and adolescents, but its presence can be noticed at any stage of growth [1]. The Cobb angle is one of the most commonly used methods to quantify the severity of scoliosis on X-rays, providing an essential standardized parameter for the assessment and management of spinal curvature [2]. However, the measurement of the Cobb angle is not without limitations. One of the main issues is inter- and intra-observer variability, which can affect measurement accuracy [3,4]. Factors such as the quality of the radiographic image, patient positioning and the physician's experience can contribute to differences in measurements, generally accepted up to 5 degrees of variation.

LiDAR (Light Detection and Ranging) technology is a remote sensing method that uses laser light to measure relative distances and produce accurate three-dimensional representations of objects or surfaces [5]. In the evaluation of scoliosis, LiDAR offers significant potential advancements over traditional methods, such as X-rays, both in terms of safety, given the absence of ionizing radiation and for its precision in representing the body's three-dimensional structure. In this context, Spine3D (Sensor Medica, Guidonia Montecelio, Italy) emerges as an innovative tool for evaluating the spine and its rotation [6].

The process of assessing scoliosis with LiDAR involves emitting laser pulses from a scanning device. These pulses reflect off the surfaces of the patient's body and return to the sensor. By analyzing the time taken for the pulses to return, the LiDAR system calculates the distance with high precision, thus constructing a three-dimensional map of the analyzed surface. These data can be used to determine the shape of the spine and other critical anatomical aspects in the diagnosis of scoliosis.

The aim of this study is to evaluate the accuracy and reproducibility of Spine3D in the measurement of the Cobb angle in patients with idiopathic scoliosis.

Methodology

This study was conducted at the Sant'Andrea University Hospital in Rome, within the Orthopedics and Traumatology Department, from September 2022 to September 2024. Patients included were those with idiopathic scoliosis aged between 10 and 18 years, with a Cobb angle between 10° and 45°. Patients with a secondary scoliotic curve, a history of vertebral fractures or the presence of cardiovascular or metabolic diseases such as obesity were excluded.

Parents or legal guardians and adolescents provided their informed consent both verbally and in writing. All procedures were in accordance with the Declaration of Helsinki (1975) as revised in 2013 [7]. Body mass was measured barefoot and in light clothing, standing upright in the center of the scale platform (Seca, Hamburg, Germany) with hands at the sides. Height was measured using a Harpenden stadiometer (Holtain Ltd., Cross-Well, UK) with a fixed vertical backboard and an adjustable head piece. The measurement was conducted with subjects in an upright position, without shoes and the head in the horizontal plane. Two measurements were taken for each parameter and a third was conducted if there was a discrepancy of 500 g and 0.5 cm between the initial measurements. The anthropometric parameters were then based on the average of the two closest measurements.

The Body Mass Index (BMI) of the patients was also assessed, calculated as $BMI = \text{weight in kilograms} / (\text{height in meters} \times \text{height in meters})$.

SPINE3D

The Spine3D® (Fig. 1) is an innovative and non-invasive three-dimensional optoelectronic detection system (Kinect) that allows for accurate assessment of vertebrae alignment. The Spine3D system consists of a single vertical aluminum panel measuring 165 × 63 × 76 cm, a 27" touchscreen monitor with a resolution of 1920 × 1080 @60Hz (2.1-megapixel Full HD) in a 16:9 vertical orientation, with dimensions LxH: 597.6 × 336.15 mm, 23.5 × 13.2".

The system uses infrared cameras called "Time of Flight" (ToF) that allow the measurement of light reflection (camera-subject-camera) without the need for a dark room. It features an RGB camera with a resolution of 1600 × 1200 pixels, a frame rate of 15 fps and a field of view of H-70° V-50°. There is also a Depth camera with a resolution of 640 × 480 pixels, a frame rate of 15 fps and a field of view of H-60° V-45°.

The internal software, using a class I infrared light beam, captures the image of the back and records the difference between the projected and acquired image, which is displayed on a panel. The data obtained from surface irregularities, automatically identified by the instrument such as the prominent vertebra, right and left shoulder and left and right lumbar dimple, are mathematically analyzed to map the spine's morphology with a three-dimensional rendering (resolution of 1 mm). All measurements were conducted in the afternoon in the same clinical office, with a constant temperature of 21°C. Participants stood barefoot on the stabilometric platform, in a quiet and upright position, with their back exposed and facing the Spine 3D, positioned approximately 110 cm away from the subjects. Measurements were taken by two different operators at a 5-minute interval.

Once the patient was correctly positioned, the exam was initiated and from that moment the patient had to remain still for 10 seconds and wait for the acquisition to be completed.

The Spine3D system identifies the following anatomical landmarks (Fig. 2):

- VP (Vertebra Prominent) = identifies the prominent vertebra, representing C7
- SL (Left Shoulder) and SR (Right Shoulder) = identify the left shoulder acromion and right shoulder acromion, respectively
- DL (Left Dimple) and DR (Right Dimple) = identify the left and right lumbar dimples, respectively, representing the posterior iliac crests of the pelvis
- SP (Sacral Prominent) = identifies the sacral prominence, representing S2-S3

Once the acquisition is complete, the software will automatically generate a patient report that includes all the values and indices of the spine. The measurements considered in this study are: the kyphotic angle, lordotic angle, shoulder disparity, pelvic tilt and the curvature angle of the spine (Fig. 3,4).



Figure 1: Spine3D.



Figure 2: Registration of anatomical landmarks during image acquisition: VP, SL, SR, DL, DR, SP.



Figure 3: Measurements performed by Spine3D in the sagittal projection of the spine.

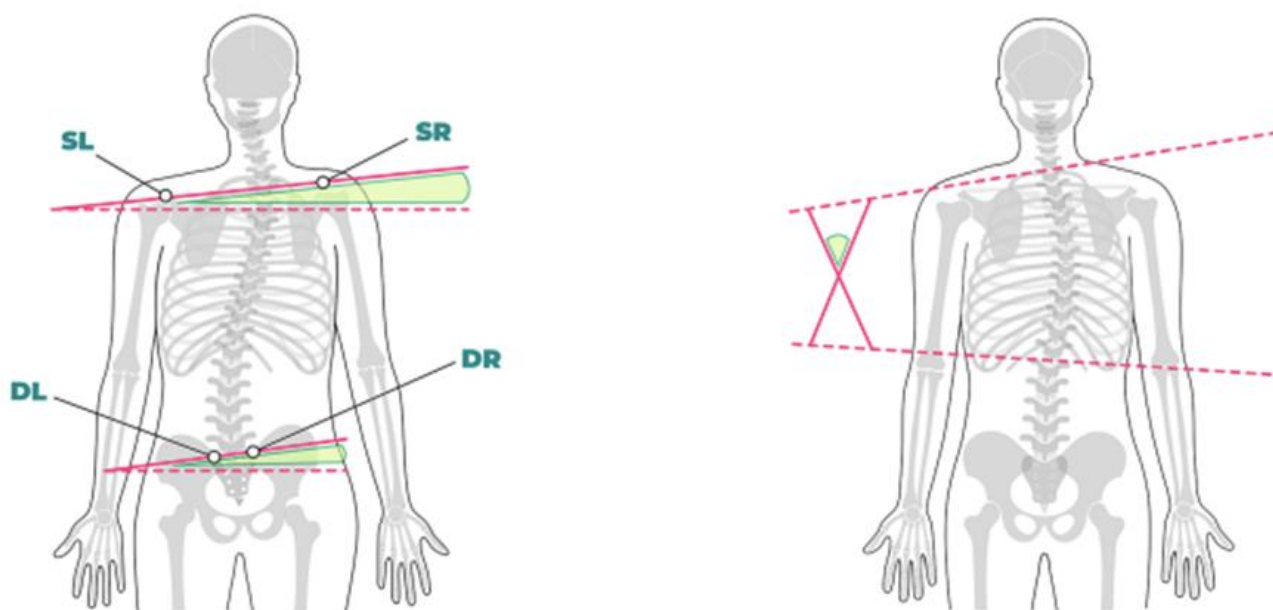


Figure 4: Measurements performed by Spine3D in the coronal projection of the spine.

Kyphotic Angle (KA) is defined as the angle formed by the tangents to the surface at the Cervico-Thoracic Inversion point (ICT) and the Thoraco-Lumbar Inversion point (ITL). It is expressed in degrees. Lordotic Angle (LA) is defined as the angle formed by the tangents to the surface at the Thoraco-Lumbar Inversion point (ITL) and the lumbo-sacral inversion point (ILS). It is expressed in degrees.

The shoulder asymmetry is assessed by the distance between the horizontal axis passing through the left acromion (SL) and the horizontal axis passing through the right acromion (SR). It is expressed in millimeters (mm). The pelvic tilt is assessed by the distance between the horizontal axis passing through the left Dimple (DL) and the horizontal axis passing through the right Dimple (DR). It is expressed in millimeters (mm).

The curvature angle is defined as the angle formed by the two tangents passing above the upper end vertebral body and below the lower end vertebral body. It is expressed in degrees.

Statistical Analysis

All data were expressed as mean, followed by $\pm$ Standard Deviation (SD), with the range of measurements in parentheses. Differences in the two measurements of the Cobb angle using Spine3D were considered. The frequency and cumulative percentage distribution of the intra-observer differences were recorded. Statistical analyses were performed using SPSS 13.0 software (SPSS Inc., Chicago, IL).

Results

The study included 29 adolescents with idiopathic scoliosis; 2 were excluded due to behavioral disorders and one did not complete the follow-up. The sample therefore consisted of 26 adolescents, whose demographic data are presented in Table 1.

Patients (n)	26
Male (n)	15
Female (n)	11
Age (anni)	13.7 $\pm$ 2.2 (10-18)
Height (m)	1.56 $\pm$ 0.1 (1.41-1.79)
Weight (Kg)	47.8 $\pm$ 8.9 (32-70)
BMI	19.4 $\pm$ 1.9 (16-25)

Table 1: Demographics data.

The average Cobb angle measured was 29.9 degrees (range, 17-58 degrees) using Spine3D. The average Cobb angles measured, the Standard Deviation (SD) between the two measurements and the 95% confidence interval for the difference between the two measurements are summarized in Table 2.

	Measurement 1	Measurement 2
Cobb Angle, mean	30.1	29.8
Cobb Angle, SD	1.1	1.4
SD of difference between 2 measurements	1.1	1.2
95% confidence interval for the difference ($\pm$) between 2 measurements	2.1	2.3

Table 2: Summary of data for the Spine3D measurement.

All other measurements are outlined in Table 3 and none proved to be statistically significant.

	Spine3D Measurements
Shoulder asymmetry (mm)	6.1 $\pm$ 1.2 (1-9)
Pelvic tilt (mm)	2.4 $\pm$ 1.3 (1-9)
Kyphotic angle (degree)	28.3 $\pm$ 2.7 (12-37)
Lordotic angle (degree)	38.41 $\pm$ 3.2 (32-44)

Table 3: The Spine3D measurement is expressed as the average of the two different measurements.

Discussion

The study highlights that Spine3D is a valid and reproducible method for the evaluation in patient with idiopathic scoliosis. Although a low-dose solution has been recently developed (EOS Imaging System, EOS Imaging, Paris, France), the ability to utilize radiation-free methods to monitor scoliosis and its progression would be advantageous [8-10]. Numerous systems based

on dorsal surface topography have been developed as non-invasive alternatives to traditional radiography (such as the Moiré projection, laser scanning, electromagnetic topography, ultrasound imaging and rasterstereography [8-26]. Based on the reconstruction of the body's back surface, these systems provide an indirect measurement of spinal deformities. Since they do not characterize the internal shape of the spine, such techniques cannot inherently diagnose the degree of scoliosis. However, the use of Artificial Intelligence (AI) has allowed the inclusion of numerous subjects to predict the anatomical conformation of the spine. Additionally, they can potentially be exploited as cost-effective and quick methods for the initial screening of spinal deformities.

Encouraging results have been reported in terms of reliability (the repetition of a measure) and validity (the measure accurately corresponding to reality).

This study represents the first utilization in the literature of a LiDAR method in idiopathic scoliosis, with certainly encouraging results. However, it has some limitations: the sample size is small, due to the strict inclusion criteria. More severe curvatures are often associated with the patient's inability to perform the test while standing and are frequently linked to secondary conditions. Additionally, the study does not consider other radiographic parameters, which could not be compared with Spine3D. Moreover, monitoring of scoliosis curvature was not performed on the patients, as this would have required additional follow-up time.

Conclusion

In conclusion, the measurement of the Cobb angle using Spine3D has demonstrated excellent reliability and efficiency. It is therefore suggested to promote the use of this method in clinical practice, alongside radiographic monitoring. Further studies will be needed to evaluate the spinal curvatures measured using Spine3D and traditional radiology.

Conflict of Interests

The authors declare that they have no conflict of interest in this paper.

Funding

None

Authors' Contributions

All authors contributed equally in this paper.

References

1. Kleinberg S. The operative treatment of scoliosis. *Arch Surg.* 1922;5:631-645.
2. Cobb JR. Outline for the study of scoliosis. In: Edwards JW, editor. *AAOS, Instructional Course Lectures.* Ann Arbor: The American Academy of Orthopaedic Surgeons; 1948;5:261-75.
3. Morrissy RT, Goldsmith GS, Hall EC, Kehl D, Cowie GH. Measurement of the Cobb angle on radiographs of patients who have scoliosis. Evaluation of intrinsic error. *J Bone Joint Surg Am.* 1990;72(3):320-7.
4. Carman DL, Browne RH, Birch JG. Measurement of scoliosis and kyphosis radiographs. Intraobserver and interobserver variation. *J Bone Joint Surg Am.* 1990;72(3):328-33.
5. Bassani T, Stucovitz E, Galbusera F, Brayda-Bruno M. Is rasterstereography a valid noninvasive method for the screening of juvenile and adolescent idiopathic scoliosis? *Eur Spine J.* 2019;28(3):526-35.
6. Marin L, Lovecchio N, Pedrotti L, Manzoni F, Febbi M, Albanese I, et al. Acute effects of self-correction on spine deviation and balance in adolescent girls with idiopathic scoliosis. *Sensors.* 2022;22(5):1883.
7. World Medical Association Declaration of Helsinki: Ethical principles for medical research involving human subjects. *JAMA.* 2013;310:2191-4.
8. Dietrich TJ, Pfrmann CW, Schwab A, Pankalla K, Buck FM. Comparison of radiation dose, workflow, patient comfort and financial break-even of standard digital radiography and a novel biplanar low-dose X-ray system for upright full-length lower limb and whole spine radiography. *Skelet Radiol.* 2013;42(7):959-67.
9. Illes T, Somoskeoy S. The EOS imaging system and its uses in daily orthopaedic practice. *Int Orthop.* 2012;36(7):1325-31.
10. Somoskeoy S, Tunyogi-Csapo M, Bogyo C, Illes T. Accuracy and reliability of coronal and sagittal spinal curvature data

- based on patient-specific three-dimensional models created by the EOS 2D/3D imaging system. *Spine J.* 2012;12(11):1052-9.
11. Aroeira RM, de Las Casas EB, Pertence AE, Greco M, Tavares JM. Non-invasive methods of computer vision in the posture evaluation of adolescent idiopathic scoliosis. *J Bodyw Mov Ther.* 2016;20(4):832-43.
 12. Prowse A, Pope R, Gerdhem P, Abbott A. Reliability and validity of inexpensive and easily administered anthropometric clinical evaluation methods of postural asymmetry measurement in adolescent idiopathic scoliosis: a systematic review. *Eur Spine J.* 2016;25(2):450-66.
 13. Porto F, Gurgel JL, Russomano T, Farinatti Pde T. Moire topography: characteristics and clinical application. *Gait Posture.* 2010;32(3):422-4.
 14. Willner S. Moire topography for the diagnosis and documentation of scoliosis. *Acta Orthop Scand.* 1979;50(3):295-302.
 15. Hill DL, Berg DC, Raso VJ, Lou E, Durdle NG, Mahood JK, et al. Evaluation of a laser scanner for surface topography. *Stud Health Technol Inf.* 2002;88:90-4.
 16. Treuillet S, Lucas Y, Crepin G, Peuchot B, Pichaud JC. SYDESCO: a laser-video scanner for 3D scoliosis evaluations. *Stud Health Technol Inf.* 2002;88:70-3.
 17. Knott P, Mardjetko S, Nance D, Dunn M. Electromagnetic topographical technique of curve evaluation for adolescent idiopathic scoliosis. *Spine (Phila Pa 1976).* 2003;31(24):E911-5.
 18. Zheng R, Chan AC, Chen W, Hill DL, Le LH, Hedden D, et al. Intra- and inter-rater reliability of coronal curvature measurement for adolescent idiopathic scoliosis using ultrasonic imaging method-a pilot study. *Spine Deform.* 2015;3(2):151-8.
 19. Cheung CW, Zhou GQ, Law SY, Mak TM, Lai KL, Zheng YP. Ultrasound volume projection imaging for assessment of scoliosis. *IEEE Trans Med Imaging.* 2015;34(8):1760-8.
 20. Manca A, Monticone M, Cugusi L, Doria C, Tranquilli-Leali P, Deriu F. Back surface measurements by rasterstereography for adolescent idiopathic scoliosis: from reproducibility to data reduction analyses. *Eur Spine J.* 2018;27(9):2130-8.
 21. Mohokum M, Schulein S, Skwara A. The validity of rasterstereography: a systematic review. *Orthop Rev (Pavia).* 2015;7(3):589-925.
 22. Drerup B. Rasterstereographic measurement of scoliotic deformity. *Scoliosis.* 2014;9(1):22.
 23. Zubovic A, Davies N, Berryman F, Pynsent P, Quraishi N, Lavy C, et al. New method of scoliosis deformity assessment: ISIS2 system. *Stud Health Technol Inf.* 2008;140:157-60.
 24. Liu XC, Thometz JG, Lyon RM, Klein J. Functional classification of patients with idiopathic scoliosis assessed by the Quantec system: a discriminant functional analysis to determine patient curve magnitude. *Spine (Phila Pa 1976).* 2001;26(11):1274-8.
 25. Goldberg CJ, Kaliszer M, Moore DP, Fogarty EE, Dowling FE. Surface topography, Cobb angles and cosmetic change in scoliosis. *Spine (Phila Pa 1976).* 2001;26(4):E55-63.
 26. Weisz I, Jefferson RJ, Turner-Smith AR, Houghton GR, Harris JD. ISIS scanning: a useful assessment technique in the management of scoliosis. *Spine (Phila Pa 1976).* 1988;13(4):405-8.

Journal of Orthopaedic Science and Research



Publish your work in this journal

Journal of Orthopaedic Science and Research is an international, peer-reviewed, open access journal publishing original research, reports, editorials, reviews and commentaries. All aspects of orthopaedic health maintenance, preventative measures and disease treatment interventions are addressed within the journal. Orthopaedicians and other researchers are invited to submit their work in the journal. The manuscript submission system is online and journal follows a fair peer-review practices.

Submit your manuscript here: <https://athenaeumpub.com/submit-manuscript/>